Accessory Kit

Application

- 1. Slip elastic loop over foot portion of orthosis. See figure A.
- 2. Slide pocket of calf liner over top of orthosis. See figure B.
- 3. Slide anklet into position over foot portion of orthosis and line up dial screw with hole provided. See figure C.
- 4. Secure anklet to back of orthosis with hook & loop tabs. See figure D.
- 5. Attach toe post cover and slide to post into dial screw at bottom of orthosis.

Washing Instructions:

Hand wash and air dry liner.

MANUFACTURER'S WARNING:


- 1. MPO 2000 requires a physician order.
- 2. Cross contamination can result when used by more than one patient.
- 3. Ambu-Assist required during ambulation or gait training for safety.
- 4. Multiple patient use of MPO 2000, alteration, or removal/substitution of parts voids manufacturer's warranty.
- 5. The MPO 2000 should only be applied by a person instructed in proper application.
- 6. Discontiinue use if redness or edema occurs and consult a physician.


Limited Warranty Coverage: Any defect in material or workmanship solely limited to the Kydex® plastic frame or metal portion or hinge mechanisms for 1 (one) year from date of purchase,







04/12 Literature may not reflect current manufacturer specifications.












Restorative Care of America

Phone: (727) 573-1595 or (800) 627-1595 Fax: (727) 573-1886 or (800) 545-7938 12221 33rd Street N, St Petersburg, FL 33716 www.rcai.com

Literature may not reflect current

MPO 2000® OIMP MPO 2000® Active OZMP

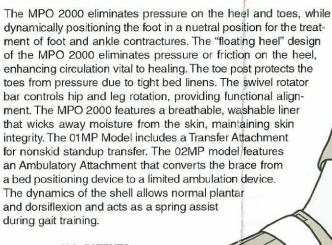






Size	Measure F	Foot Length	Max Calf Circ.		Transfer Attachment Model #	Ambulatory Attachment Model #
Infant	3 - 4" (7.6 - 10.2 cm)		8" (20.3 cm)		01MP-I	-
Toddler	4 1/2 - 6"	(11.4 - 15.2 cm)	10"	(25.4 cm)	01MP-T	-
Child	5 – 7"	(12.7 - 17.8 cm)	10"	(25.4 cm)	01MP-C	-
Youth	6 1/2 - 9"	(16.5 - 22.9 cm)	13"	(33 cm)	01MP-Y	77
Small	7 – 8"	(17.8 - 20.3 cm)	15"	(38.1 cm)	01MP-S	02MP-S
Medium	8 - 9"	(20.3 - 22.9 cm)	17"	(43.2 cm)	01MP-M	02MP-M
Large	9 - 10"	(22.9 - 25.4 cm)	17"	(43.2 cm)	01MP-L	02MP-L
Ex. Large	10 - 11"	(25.4 - 27.9 cm)	18"	(45.7 cm)	01MP-XL	02MP-XL
XX Large	11 -12 1/2	" (27.9 – 31.8 cm)	18"	(45.7 cm)	01MP-XXL	-

Limited Warranty Coverage: Any defect in material or workmanship solely limited to the Kydex® plastic frame or metal portion or hinge mechanisms for 1 (one) year from date of purchase.


Application of the MPO 2000®




Bend knee and seat foot firmly in orthosis. Press with palm over instep.




Fold calf liner around calf and secure in place.




Smoothly fold anklet over instep.



Check clearance below heel. Check that sole of foot makes contact with the orthosis.



Secure anklet with hook & loop strap provided.



Avoid this position. (Repeat steps #1-5).



Patient Problem

CARE PLAN

- 1) Foot drop, foot/ankle contractures.
- 2) Internal/external rotation of foot and/or ankle.
- 3) Fx hip, post fx hip, internal rotation or scissoring of extremities.
- 4) Pressure uicers of foot, ankle, toes or heel.

Expected Outcome

- 1) Correct foot drop or foot/ankle contractures.
- 2) Correct internal/external rotation of the foot and/or ankle.
- 3) Maintain functional alignment of foot/ankle.
- 4) Prevent permanent deformity.
- 5) Abduction of lower extremities to maintain functional alignment.
- 6) Eliminate pressure to effected area.

Nursing Actions

- 1) Passive range of motion to foot and/or ankle Q8H or as prescribed.
- 2) Treatment per physician's orders.
- 3) Apply orthosis as per instructions inside.
- 4) Check for correct positioning of orthosis at heel Q2H.
- 5) Position rotator bar to correct internal or external rotation.
- 6) Attach spreader bar to bilateral rotator bars to maintain abduction
- 7) Remove Q8H or per physician or therapy order.
- 8) Document progress in chart.

Nursing Alert

- Wearing time may be increased according to patient's tolerance and response.
- 2) Clearance should be observed below heel. Sole of foot should be in contact with orthosis.



Restorative Care of America

Phone: (727) 573-1595 or (800) 627-1595 Fax: (727) 573-1886 or (800) 545-7938 12221 33rd Street N, St Petersburg, FL 33716 www.rcal.com

05/16

Literature may not reflect current manufacturer specifications.



Ambulatory Attachment 02AA

RCAI's Ambulatory Attachment provides a non-skid, rocker bottom walking platform for the Multi Podus® System during stand up transfer and ambulation.

The Ambulatory Attachment requires no tools for application or removal. The one piece combination foot plate, toe post and rubber sole design of the attachment easily locks in place over the toe post dial of the Multi Podus® System for security and safety.

In use, the Ambulatory Attachment becomes an ambulation device for gait training. When detached, cross contamination from floor to bed is avoided assuring compliance with infection control standards.


TO APPLY:


- 1. Position attachment perpendicular to bottom of Multi Podus® System. Align round "key hole" portion of attachment over the toe post dial of splint, and press down with thumb. (Fig 1)
- 2. Slide attachment until the toe post dial locks in position at end of slot. (Fig 2)
- Holding the bottom heel portion of attachment, rotate toward bottom of splint to position. (Fig 3)


Secure velcro tabs on the Ambulatory Attachment to velcro tabs sewn on liner.

TO REMOVE: Lift heel portion of attachment to disengage velcro tabs. Rotate attachment until perpendicular to splint and slide until toe post dial is aligned with round "key hole". Lift attachment over toe post and remove.

NOTE: The toe post dial must be loosened all the way out before reapplying the Ambulatory Attachment.







Limited Warranty Coverage: Any defect in material or workmanship solely limited to the Kydex® plastic frame or metal portion or hinge mechanisms for 1 (one) year from date of purchase.